



FIG. 1

09765821.042301

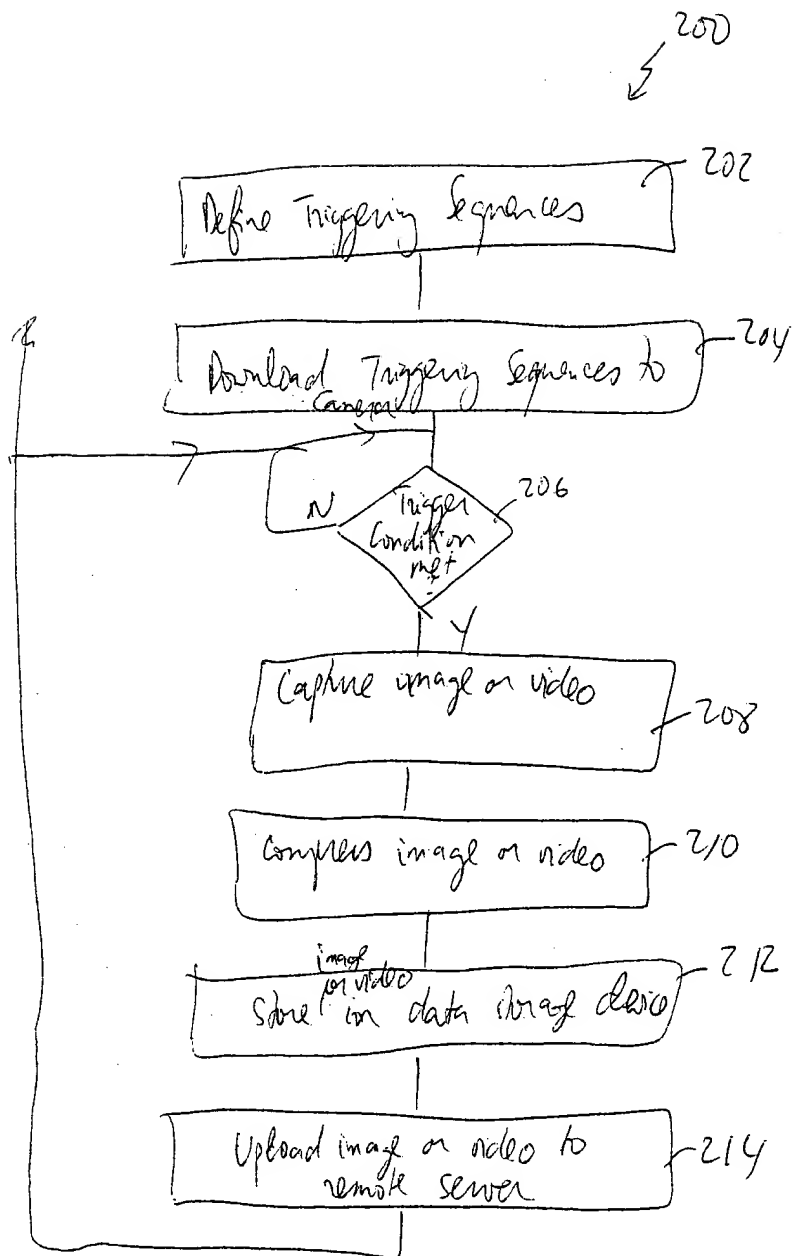

F. 2

09765821.042301

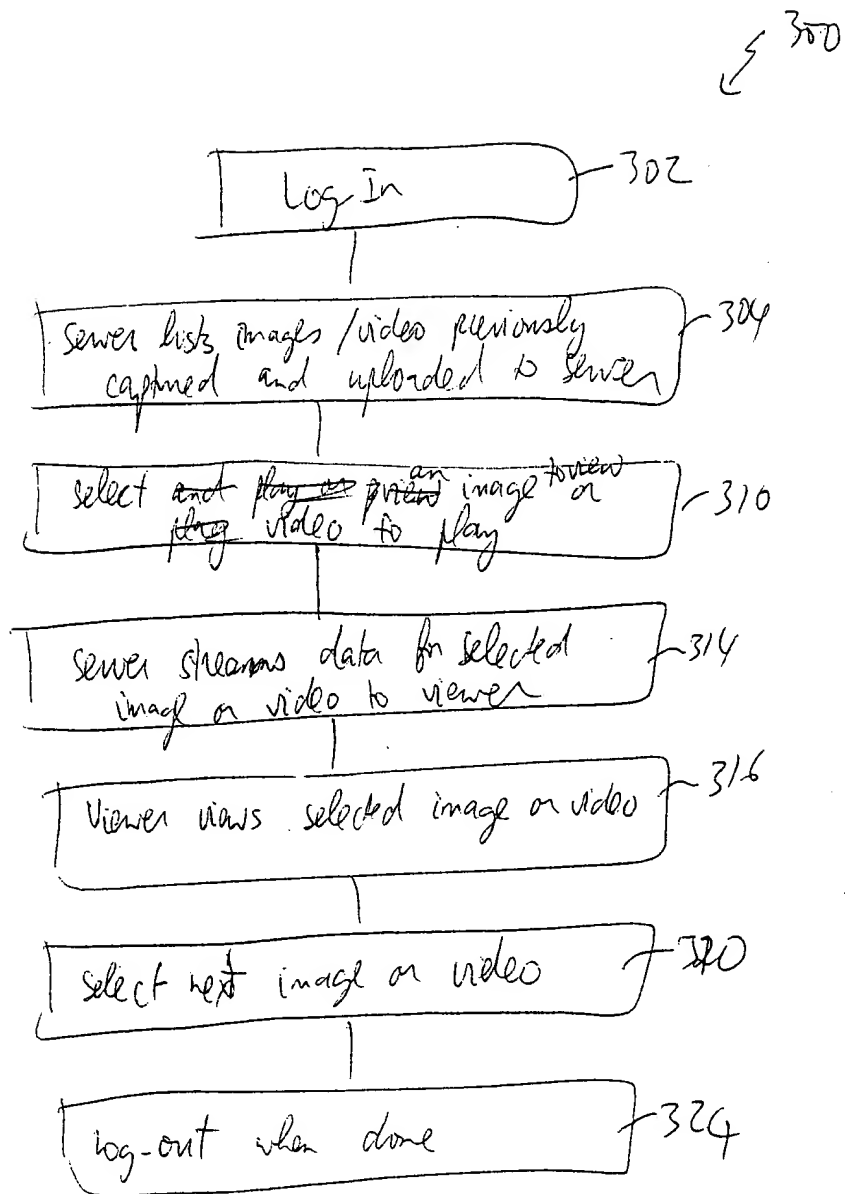

F.3

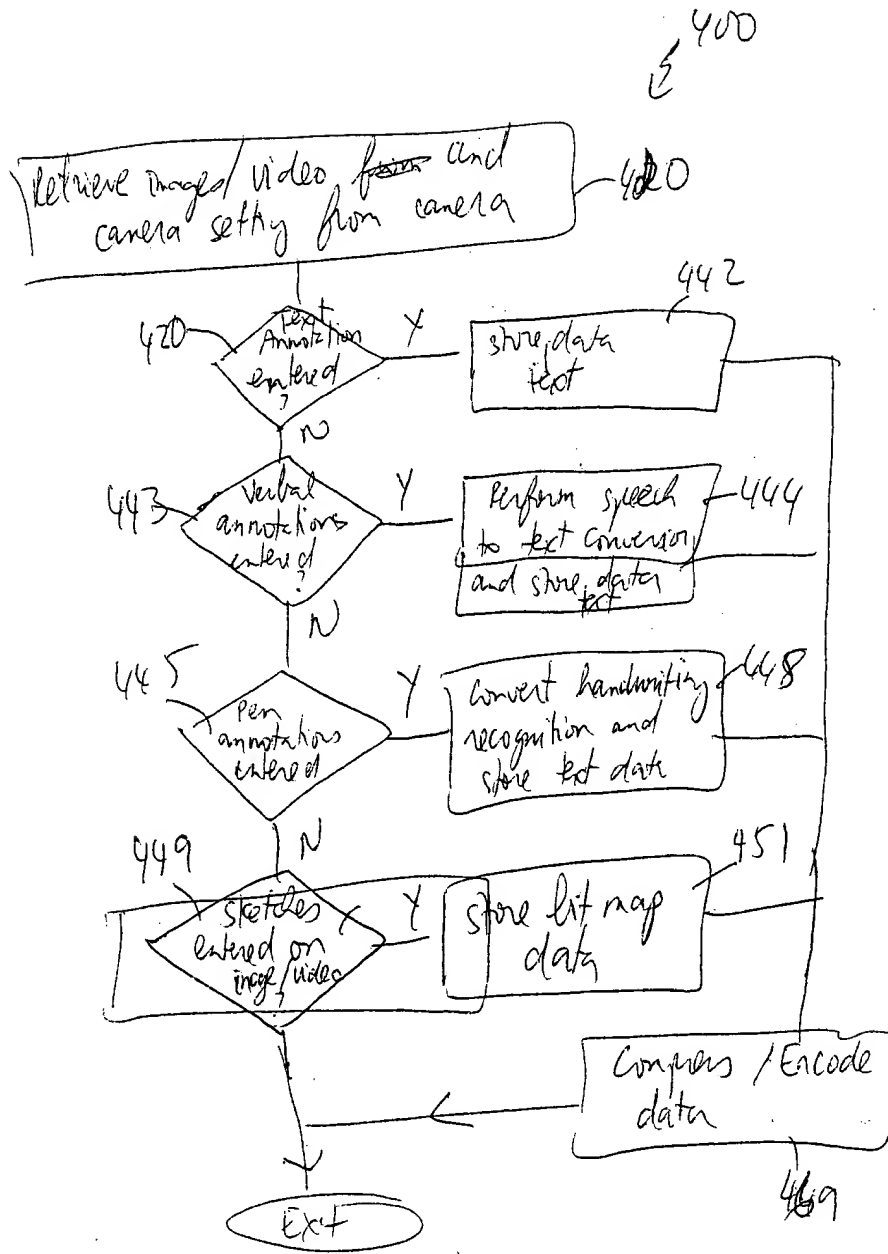


Fig. 4



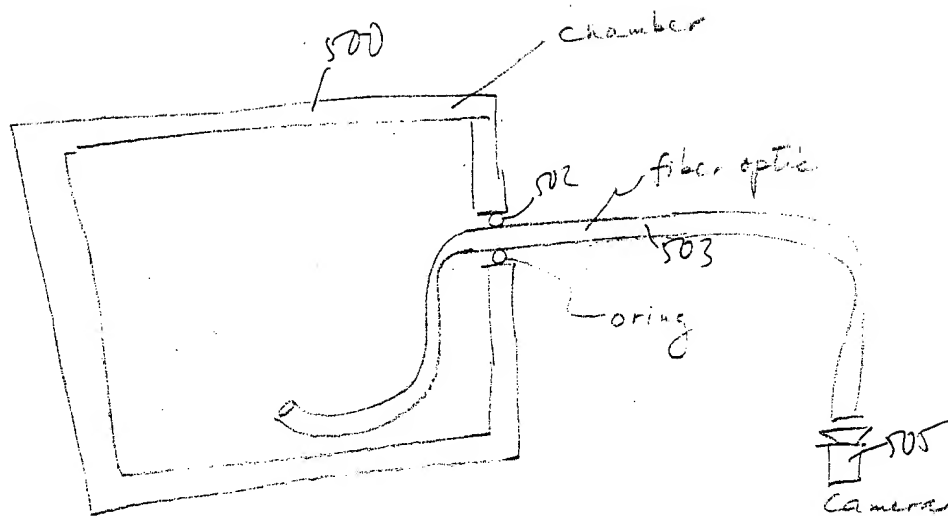


Fig 5.
Vacuum adapter for viewing inside the
chamber

09765821.04301

09765821.042301

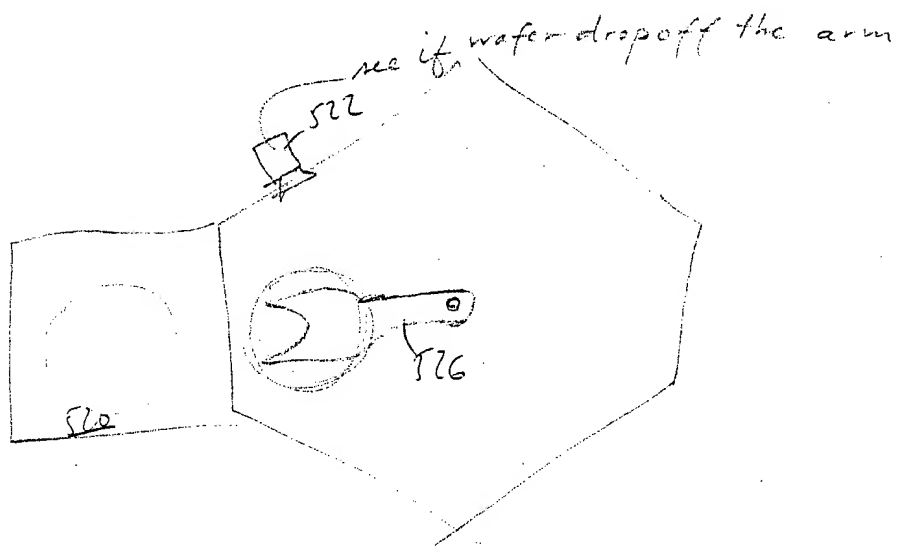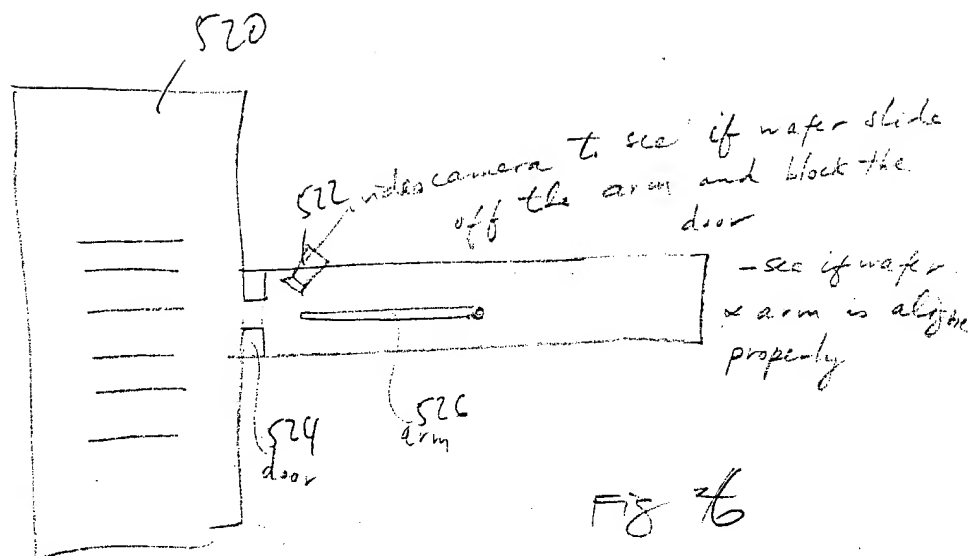

09765821.042301

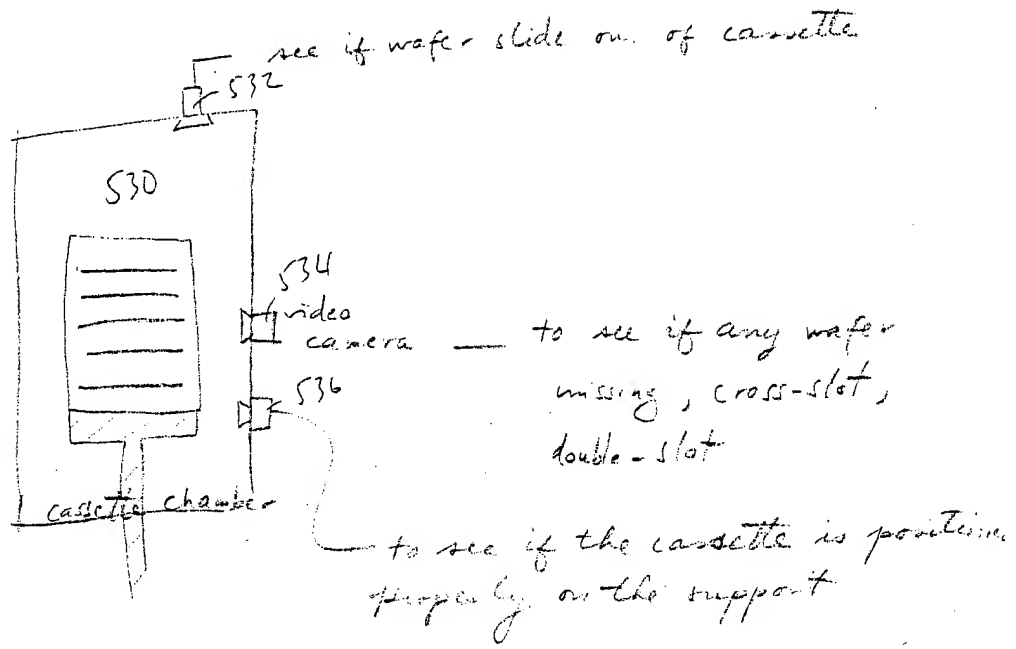


Fig 8

09765821.042301

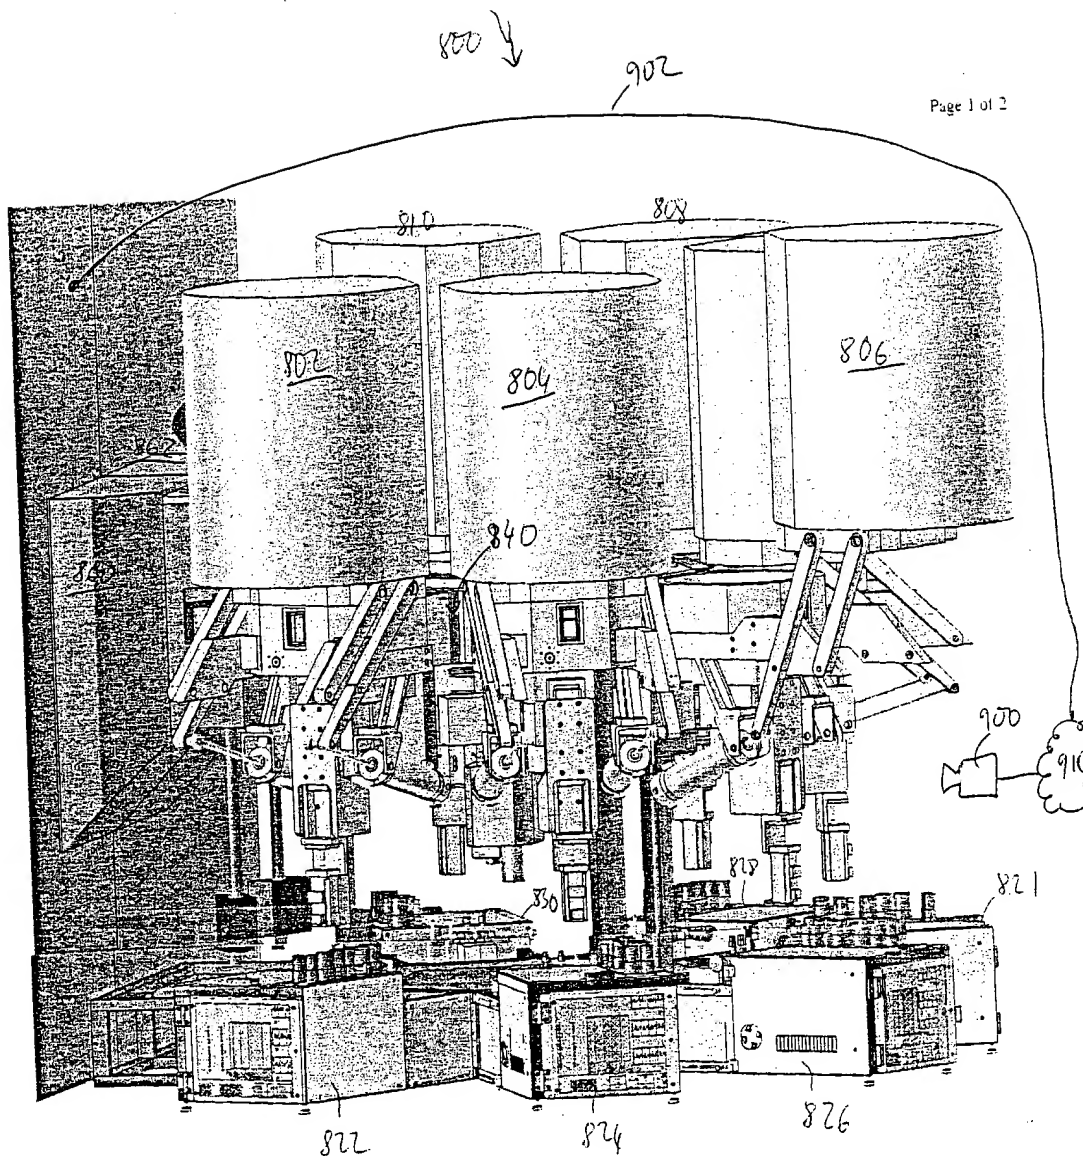


FIG. 9